


# WOODPEX 1 APEX LOCATOR



## Woodpex I Apex Locator Instruction Manual

(Please read this manual before operating)

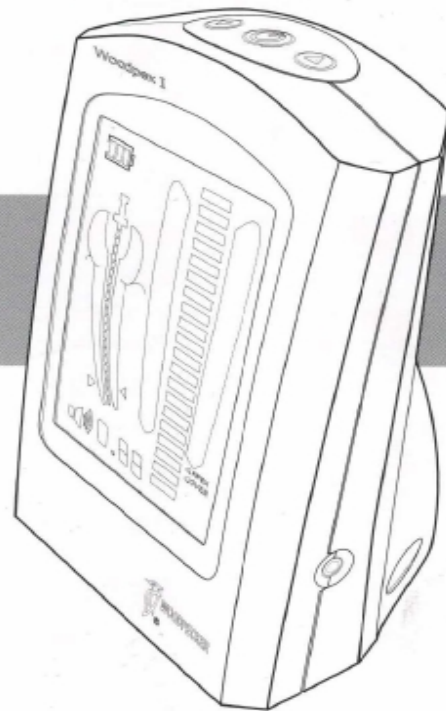

Certificated  
**CE 0197**  
EN ISO 9001:2008  
EN ISO 13485:2003+A1:2007

**Guilin Woodpecker Medical Instrument Co., Ltd.**

1		1
2		1
3		1
4		1
5	( )	3
6		3
7		3
8		5
9		6
10		6
11		8
12		8
13		9
14		10
15		10
16		11
17		12
18		12
19		12

1. \_\_\_\_\_

WOODPEX 1

2. \_\_\_\_\_

85 ( ) 74 ( ) 121 ( )

3. \_\_\_\_\_

, ; , ; .

4. \_\_\_\_\_


WOODPEX 1 :

- 
- 
- 
- 
-



# Woodpex I Apex Locator Instruction Manual

(Please read this manual before operating)

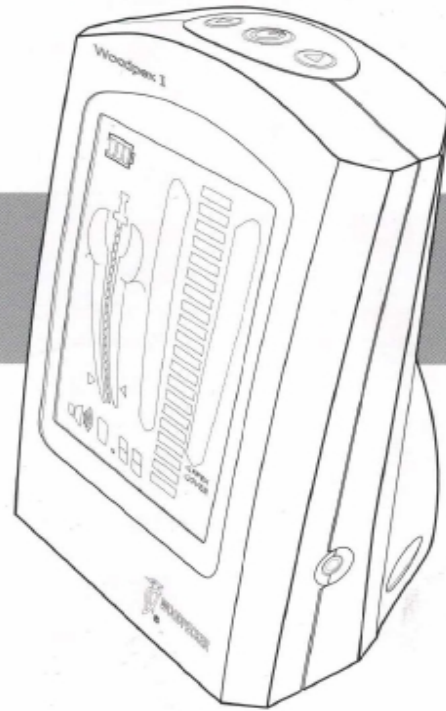


Certificated  
**CE 0197**  
EN ISO 9001:2008  
EN ISO 13485:2003+AC:2007

**Guilin Woodpecker Medical Instrument Co., Ltd.**

.1 :

- Power indicator –
- Power on/off – /
- Sound adjustment –
- Length measure indicator –
- Sound indicator –
- Emulsion of enlarging apex –
- Measuring wire socket -

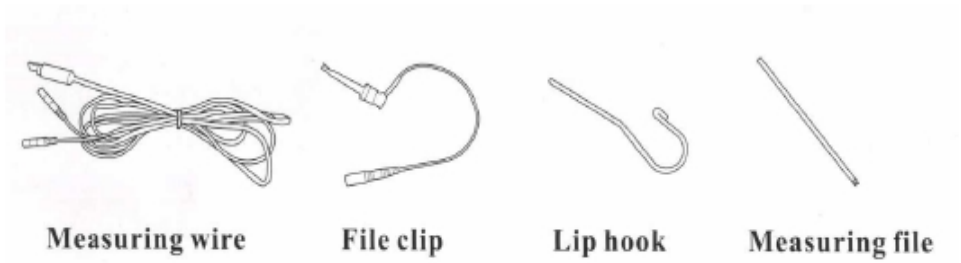

Measuring wire

File clip

Lip hook

Measuring file

5. \_\_\_\_\_ :

Measuring wire -

File clip -

Lip hook -

Measuring file -

6. \_\_\_\_\_

( ), ( , . . ) (

7. \_\_\_\_\_ .

7.1.

7.2.

7.3.

7.4.

7.5.

7.6.

7.7.

7.8. :4 LR03, 1,5

7.9.

7.10.

7.11.

7.12.

7.13.

8.

8.1 -

8.2

8.3.

8.4. -

8.5.

8.6.

9. \_\_\_\_\_.

9.1.

9.2.

9.3. (4 )

10 \_\_\_\_\_

10.1.

10.2.


10.3.

10.4.

10.5.

2 , . . . .2

picture 2

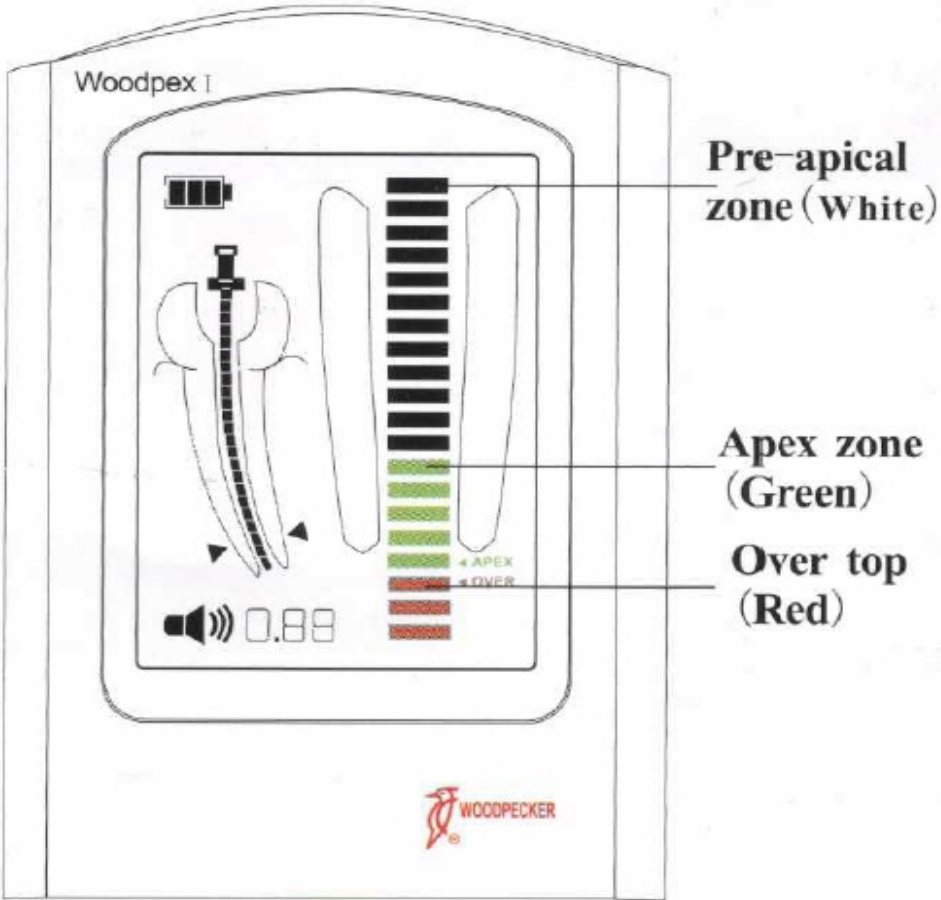

( - - )  
10.6.

10.7.

75%

11. \_\_\_\_\_

- 11.1. : (4 )
- 11.2. : 0,5 W
- 11.3. : 3.2", (LCD)
- 11.4. :  
2 .

12. \_\_\_\_\_

- 12.1. (4 )
- 12.2. : BF
- 12.4. , .
- 12.5.
- 12.6.
- 12.7. :

13. \_\_\_\_\_

**WOODPECKER** Trademark

Use indoor only

Consult instructions for use

**IPX0** Ordinary equipment, not protect against ingress of water

Sound adjustment

Type BF applied part

Manufacturer

Self-check on/off

Caution, consult accompanying documents

Date of manufacture

Power on/off

Temperature limitation: -10°C to +50°C

Humidity limitation: 0% to 100%

Atmospheric pressure for storage: 50 to 106

EC REP

Authorised Representative in the EUROPEAN COMMUNITY

Appliance compliance WEEE directive

**CE 0197** CE mark

**EN ISO 9001:2008** Certificated by international quality control system of ISO

**EN ISO 13485:2003+AC:2007** Certificated by medical instrument manufacturer quality control system of ISO



- 1)
- 2)IPXO -
- 3) BF:
- 4) :
- 5)
- 6)
- 7)
- 8)
- 9)
- 10)
- 11)
- 12) -
- 13)
- EN ISO 9001:2008 -
- EN ISO 13485:2003+AC:2007 -

- 14) .
- 15)
- 16) /
- 17) /

14. \_\_\_\_\_

14.1.

14.2

14.3. .( , 135 )

14.4.

14.5.

14.6.

14.7.

15.

15.1

15.2

15.3.

16.

16.1.

16.2.

16.3.

16.4.

. :  
. : -10 +50  
. : 80%  
. 50 - 106

17.

18. \_\_\_\_\_

EC REP

Wellkang Ltd ([www.CE-marking.eu](http://www.CE-marking.eu))

29 Harley St., London W1G 9QR, UK ( )

19. \_\_\_\_\_

19.1 2

6

19.2.